

FORM PTO-1390  
(REV 12-29-99)

U.S. DEPARTMENT OF COMMERCE PATENT AND TRADEMARK OFFICE

ATTORNEY'S DOCKET NUMBER

TRANSMITTAL LETTER TO THE UNITED STATES  
DESIGNATED/ELECTED OFFICE (DO/EO/US)  
CONCERNING A FILING UNDER 35 U.S.C. 371

U.S. APPLICATION NO. (If known, see 37 CFR 1.5)

09/509377

INTERNATIONAL APPLICATION NO.  
PCT/LV 98/00006INTERNATIONAL FILING DATE  
October 2, 1998PRIORITY DATE CLAIMED  
October 3, 1997TITLE OF INVENTION **Endoscope with single-use cartridge for the invagination of endoscopic tube**

APPLICANT(S) FOR DO/EO/US


**Sergey Matasov, Andrei Motasov, Vita Matasova**

Applicant herewith submits to the United States Designated/Elected Office (DO/EO/US) the following items and other information:

1. ☒ This is a **FIRST** submission of items concerning a filing under 35 U.S.C. 371.
2. ☐ This is a **SECOND** or **SUBSEQUENT** submission of items concerning a filing under 35 U.S.C. 371.
3. ☒ This express request to begin national examination procedures (35 U.S.C. 371(f)) at any time rather than delay examination until the expiration of the applicable time limit set in 35 U.S.C. 371(b) and PCT Articles 22 and 39(1).
4. ☒ A proper Demand for International Preliminary Examination was made by the 19th month from the earliest claimed priority date.
5. ☒ A copy of the International Application as filed (35 U.S.C. 371(c)(2))
  - a. ☐ is transmitted herewith (required only if not transmitted by the International Bureau).
  - b. ☒ has been transmitted by the International Bureau.
  - c. ☐ is not required, as the application was filed in the United States Receiving Office (RO/US).
6. ☒ A translation of the International Application into English (35 U.S.C. 371(c)(2)).
7. ☐ Amendments to the claims of the International Application under PCT Article 19 (35 U.S.C. 371(c)(3))
  - a. ☐ are transmitted herewith (required only if not transmitted by the International Bureau).
  - b. ☐ have been transmitted by the International Bureau.
  - c. ☐ have not been made; however, the time limit for making such amendments has NOT expired.
  - d. ☐ have not been made and will not be made.
8. ☐ A translation of the amendments to the claims under PCT Article 19 (35 U.S.C. 371(c)(3)).
9. ☒ An oath or declaration of the inventor(s) (35 U.S.C. 371(c)(4)).
10. ☒ A translation of the annexes to the International Preliminary Examination Report under PCT Article 36 (35 U.S.C. 371(c)(5)).

**Items 11. to 16. below concern document(s) or information included:**

11. ☐ An Information Disclosure Statement under 37 CFR 1.97 and 1.98.
12. ☐ An assignment document for recording. A separate cover sheet in compliance with 37 CFR 3.28 and 3.31 is included.
13. ☐ A FIRST preliminary amendment.  
☐ A SECOND or SUBSEQUENT preliminary amendment.
14. ☐ A substitute specification.
15. ☐ A change of power of attorney and/or address letter.
16. ☒ Other items or information:
  1. **Certified copy of priority application P-97-190**
  2. **Certified copy of priority application P-98-188**
  3. **Copy of the author certificate № 1522466**
  4. **Copy of the International Preliminary Examination Report**

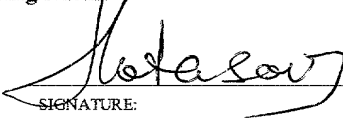U.S. APPLICATION NO. (if known, see 37 CFR 1.5) <b>09/509377</b>		INTERNATIONAL APPLICATION NO. <b>PCT/LV 98/00006</b>		ATTORNEY'S DOCKET NUMBER	
17. <input checked="" type="checkbox"/> The following fees are submitted: <b>BASIC NATIONAL FEE (37 CFR 1.492(a)(1)-(5)):</b> Neither international preliminary examination fee (37 CFR 1.482) nor international search fee (37 CFR 1.445(a)(2)) paid to USPTO and International Search Report not prepared by the EPO or JPO ..... <b>\$970.00</b> International preliminary examination fee (37 CFR 1.482) not paid to USPTO but International Search Report prepared by the EPO or JPO ..... <b>\$840.00</b> International preliminary examination fee (37 CFR 1.482) not paid to USPTO but international search fee (37 CFR 1.445(a)(2)) paid to USPTO ..... <b>\$690.00</b> International preliminary examination fee paid to USPTO (37 CFR 1.482) but all claims did not satisfy provisions of PCT Article 33(1)-(4) ..... <b>\$670.00</b> International preliminary examination fee paid to USPTO (37 CFR 1.482) and all claims satisfied provisions of PCT Article 33(1)-(4) ..... <b>\$96.00</b> <b>ENTER APPROPRIATE BASIC FEE AMOUNT =</b>				<b>CALCULATIONS</b> PTO USE ONLY	
Surcharge of <b>\$130.00</b> for furnishing the oath or declaration later than <input type="checkbox"/> 20 <input type="checkbox"/> 30 months from the earliest claimed priority date (37 CFR 1.492(e)).				\$	
CLAIMS	NUMBER FILED	NUMBER EXTRA	RATE		
Total claims	<b>10 - 20 =</b>		X <b>\$18.00</b>	\$	
Independent claims	<b>6 - 3 =</b>		X <b>\$78.00</b>	\$ <b>234.00</b>	
MULTIPLE DEPENDENT CLAIM(S) (if applicable)			+ <b>\$260.00</b>	\$ <b>260.00</b>	
<b>TOTAL OF ABOVE CALCULATIONS =</b>				\$ <b>1464.00</b>	
Reduction of 1/2 for filing by small entity, if applicable. A Small Entity Statement must also be filed (Note 37 CFR 1.9, 1.27, 1.28).				\$ <b>732.00</b>	
<b>SUBTOTAL =</b>				\$ <b>732.00</b>	
Processing fee of <b>\$130.00</b> for furnishing the English translation later than <input type="checkbox"/> 20 <input type="checkbox"/> 30 months from the earliest claimed priority date (37 CFR 1.492(f)).				\$	
<b>TOTAL NATIONAL FEE =</b>				\$ <b>732.00</b>	
Fee for recording the enclosed assignment (37 CFR 1.21(h)). The assignment must be accompanied by an appropriate cover sheet (37 CFR 3.28, 3.31). <b>\$40.00</b> per property				\$	
<b>TOTAL FEES ENCLOSED =</b>				\$ <b>732.00</b>	
				Amount to be refunded:	\$
				charged:	\$
<b>money order</b> a. <input checked="" type="checkbox"/> A <del>check</del> in the amount of \$ <u><b>732.00</b></u> to cover the above fees is enclosed.  b. <input type="checkbox"/> Please charge my Deposit Account No. _____ in the amount of \$ _____ to cover the above fees. A duplicate copy of this sheet is enclosed.  c. <input type="checkbox"/> The Commissioner is hereby authorized to charge any additional fees which may be required, or credit any overpayment to Deposit Account No. _____. A duplicate copy of this sheet is enclosed.					
<b>NOTE: Where an appropriate time limit under 37 CFR 1.494 or 1.495 has not been met, a petition to revive (37 CFR 1.137(a) or (b)) must be filed and granted to restore the application to pending status.</b>					
SEND ALL CORRESPONDENCE TO:  <b>Ranka dambis 7/1 - 55</b> <b>Riga, LV1048</b> <b>LATVIA</b>					
				 SIGNATURE:	
				NAME <b>Sergey Matasov</b>	
				REGISTRATION NUMBER	

**STATEMENT CLAIMING SMALL ENTITY STATUS  
(37 CFR 1.9(f) & 1.27(b))--INDEPENDENT INVENTOR**

Docket Number (Optional)

Applicant, Patentee, or Identifier: Sergey Matasov  
Application or Patent No.: PCT/LV 98/00006  
Filed or Issued: October 2, 1998  
Title: Endoscope with single-use cartridge for the invagination of endoscopic tube

As a below named inventor, I hereby state that I qualify as an independent inventor as defined in 37 CFR 1.9(c) for purposes of paying reduced fees to the Patent and Trademark Office described in:

- ☒ the specification filed herewith with title as listed above.  
☐ the application identified above.  
☐ the patent identified above.


I have not assigned, granted, conveyed, or licensed, and am under no obligation under contract or law to assign, grant, convey, or license, any rights in the invention to any person who would not qualify as an independent inventor under 37 CFR 1.9(c) if that person had made the invention, or to any concern which would not qualify as a small business concern under 37 CFR 1.9(d) or a nonprofit organization under 37 CFR 1.9(e).

Each person, concern, or organization to which I have assigned, granted, conveyed, or licensed or am under an obligation under contract or law to assign, grant, convey, or license any rights in the invention is listed below:

- ☒ No such person, concern, or organization exists.  
☐ Each such person, concern, or organization is listed below

Separate statements are required from each named person, concern, or organization having rights to the invention stating their status as small entities. (37 CFR 1.27)

I acknowledge the duty to file, in this application or patent, notification of any change in status resulting in loss of entitlement to small entity status prior to paying, or at the time of paying, the earliest of the issue fee or any maintenance fee due after the date on which status as a small entity is no longer appropriate. (37 CFR 1.28(b))

Sergey Matasov  
NAME OF INVENTOR  
  
Signature of inventor

\_\_\_\_\_  
NAME OF INVENTOR  
\_\_\_\_\_  
Signature of inventor

\_\_\_\_\_  
NAME OF INVENTOR  
\_\_\_\_\_  
Signature of inventor

March 20, 2000  
Date

\_\_\_\_\_  
Date

\_\_\_\_\_  
Date

4/PRB  
1

09/509377  
430 Rec'd PCT/PTO 27 MAR 2000

## **Endoscope with disposable cartridge for the invagination of endoscopic tube**

### **Description of invention**

The invention pertains to the field of medicine, namely to colonoscopy and enteroscopy, but can also be used for industrial endoscopes.

Is known the device under FGR patent No. 3329176, which includes an endoscopic tube, encased in an eversible elastic thin-walled tube which functions as a transporter-invaginator (hereinafter - invaginator) of the first tube. The invaginator in the device patented in FGR is set in long layers parallel to the transported tube. To the drawbacks of this device pertains the inconsequential unreeling of invaginator's layers which is explained by their "sticking together" due to air pressure and inevitable getting of air into spaces between them. Untimely everting of any layer excludes from participation in intubation process other layers located above the everted one.

Is known also the intestinal endoscope under the USSR author's certificate No. 1522466 with an invaginator set in short layers and placed at the right angle with an endoscopic tube, which is transported by it. This endoscope is set as a basis to the present invention and will be taken as a prototype. Endoscope-prototype comprise: - source of light; - source 5 of excessive pressure; - endoscopic tube 3 with eyepiece 1, control bloc 2 with communication branch, stop 11 for spring 10; - invaginator of endoscopic tube 3 which consists of everted part 4 and uneverted part, encased in part 4, at that, the uneverted part of invaginator tightly adjoins to an endoscopic tube and is placed in short layers perpendicularly to it. From the side of uneverted end 7 the invaginator is supported with spring 10, but the place of transition of uneverted part of the invaginator into everted 4 is limited by tip 6. Besides, the endoscope-prototype has: - external seal 13 of tube 3 on which the end 12 of the everted part 4 of invaginator is fixed with ring 16; - rings 8, 9 on the uneverted end 7 of the invaginator; - air-duct 15 with cock 17 for feeding working pressure into cavity 14 of everted part 4 of the invaginator; anal dilator 19. Apart from light and image transmission elements, biopsy channels, channels for gas or liquid supply, an endoscopic tube 3 of the prototype comprises two pairs of closely wound springs containing traction lines which pairwise connects the distal ring of a mechanism for bending the distal end of a tube and rollers for manual extraction of traction lines located in block 2.

The first drawback of the prototype is unreliable functioning of its invaginator - difficulties in introducing endoscopic tube 3 into seal 13 (see 42-53 lines of a.c. No.1522466). The invaginator is to be everted under tip 6, but during invagination the distal part of tube 3 becomes bared. It can be due both to lack of a gap between tube 3 and uneverted part of the invaginator and to a friable structure of the latter, which under the action of air pressure adheres to tube 3. Tube pleats formed during bending of the distal end also prevent free movement of the invaginator along tube 3. As a result the spring is unable to displace the invaginator to

09509377, 082800

tip 6. In addition, the invaginator's end 7, connected with two rings, ensures poor pressurization of cavity 14.

The second drawback of known endoscopes is that bending of its distal end is possible only until a definite number of flexures of an endoscopic tube. Its end is bent by rotating of two rollers each connected to its pair of traction lines. Springs, which comprise traction lines, on the distal end continue channels in the wall of cardan-joint rings. Ends of traction lines are soldered to the distal ring of the cardan mechanism for bending the distal end of the tube. Outward extraction of traction lines from the spring decreases gaps between cardan rings and forms a small radius of a flexure. Herewith, the distal cardan ring pulls the opposite traction line in distal direction, thus ensuring an increase of space between rings. Difference of lengths of big and small half-circumferences of the tube's bend is a product of « $\pi$ » and diameter of an endoscopic tube. Japanese authors point out that when 3-4 loops are formed, the distal end of an endoscope is blocked, but biopsy forceps continue to function. This difference is explained by L. Aler formula

$$\frac{Q_1}{Q_2} = e^{a \cdot f},$$

where: « $Q_1$ » - manual power realizing traction lines extraction; « $Q_2$ » - remaining from « $Q_1$ » power, attached to a distal cardan ring or cutters of biopsy forceps; « $e$ » - basis of natural logarithm; « $a$ » - traction line rotations in radians; « $f$ » - friction index between a traction line and a spring. Under fixed values « $Q_1$ » and « $f$ », value « $Q_2$ » depends on value « $a$ », but for two consecutively connected traction lines of an endoscope the latter is twice as large as for one line of biopsy forceps.

The third drawback of the prototype are problems of its maintenance. For recurrent use an endoscope is washed, disinfected and sterilized. However, there are reported cases of infecting patients with AIDS and other infections after endoscopy. Preparation of the endoscope-prototype for work also includes its assembly. The number of detached parts of this endoscope amounts to 10, but its assembly takes about half an hour. Ergonomics of operating existing endoscopes also impede its mastering. Thus, the left hand holds the control bloc, switches its cocks, rotates handles, which bend and fix the distal end of the tube, but the right hand introduces the tube into the intestine.

It has been practically proved that if an endoscope has more than 3-4 loops, it is impossible to introduce biopsy forceps into it and take biopate. This is the fourth drawback of the prototype.

The objectives of the invention have been: - increase reliability of invagination of an endoscopic tube; - ensure bending of its distal end in flexuous channels; - make maintenance of an endoscope more convenient; - perform biopsy in flexuous channels. Implementation of these objectives will make colonoscopy available to any physician and make it easier for experienced endoscopists.

These objectives have been achieved by the fact that in the composition of an endoscope, which contains: - source of light; - source of pressure; - biopsy forceps; - an endoscopic tube with the control bloc and communication branch, at that the endoscopic tube contains

005509377.082800

internally elements for light and image transmission, a channel gas/liquid, a biopsy channel, two pairs of springs with traction lines, which pairwise connect the mechanism for bending the distal end of the endoscopic tube with manual extractors of traction lines located in the control block, but externally a compressed spring placed on tubes distal end, the invaginator, the tip, a mobile seal, an anal dilator, additionally has been included:

- a new cylindrical invaginator, ensuring invagination of an endoscopic tube;
- a disposable cartridge connecting an invaginator with auxiliary elements;
- an endoscopic tube ensuring fixation of a cartridge;
- a mechanism for introduction of tube, ensuring concurrently with a cartridge insertion of a tube;
- a system of extractors-intractors of traction lines for bending the tube's end;
- a biopsy forceps' introduction and extraction system and traction line intensifier of biopsy forceps;
- a desk and pedal units of a control bloc of an endoscopic tube.

A compact hollow cylinder of the invaginator is formed of crumpled and tightly compressed in longitudinal and transverse directions short layers of different forms of an eversible thin-walled tube placed at different angles with the longitudinal axis of an endoscopic tube. The cylinder has recurrent narrowings of an external and widenings of its internal diameter.

A disposable sterile cartridge for invagination consists of a shell which has a projection at its proximal end, comprising: an invaginator; a compressed spring; its fixator; a spring distancer in which the distal seal of the endoscopic tube is located, which is joined to an uneverted end of the invaginator; a condom of the distal part of the endoscopic tube fastened at the proximal end to a spring stop, but at the distal end - to the tip with elements for hermetic joining to the endoscopic tube, at that on the shell is located a proximal seal of the endoscopic tube with the anal dilator with the channel in its wall, but at the distal end of the shell the everted end of the invaginator is fastened. In addition to elements for air-tight joining to the endoscopic tube the tip may have a protective glass and a channel for glass washing.

A novel endoscopic tube is supplemented with: - internal transverse pleats of its external cover; - two air-ducts, the larger one has a lateral opening into the cavity of the proximal seal of the disposable cartridge for invagination, but the smaller - into the cavity of distal and proximal condoms; - areas for air-tight fixation of condoms' ends; - a proximal condom.

The mechanism for introduction of the endoscopic tube consists of the cylinder with two pistons, which are interconnected with distancers and an elastic tube. The cylinder is joined with the cartridge for invagination of the endoscopic tube. The cavity between pistons and the elastic tube is connected to the source of pressure or atmosphere (vacuum) through the cock. The cavity between the distal piston and the proximal seal of the endoscopic tube is connected to the source of vacuum or atmosphere (pressure) through the cock. The cocks can be placed in the pedals but the spring, which returns pistons to their home position can be located in the cavity between the proximal seal of the endoscopic tube and the distal piston.

09509377 " 082800

The system of extraction-intraction of traction lines ensuring management over the endoscopic tube's distal end, has a hydro-manual drive and creates additional power equal to a few grams at the distal end of traction lines. The system includes sources of pressure and vacuum connected to elastic tubes containing liquid and springs with traction lines. Tubes are fixed to springs with thread, but springs are made with steps. At the distal end springs are connected with traction lines. In the control bloc traction lines are attached to manual extractors-intractors of traction lines connected to elements ensuring synchronous feeding of vacuum into the cavity of a manually extracted traction line and feeding of pressure into the cavity of an introduced traction line. At the distal end of the tube and traction line a cylinder/piston unit can be placed or a segment of sylphone, the distal end of which is connected to a traction line. A manual extractor-intractor of traction line could be made in the manner of a rod, but the sources of pressure and vacuum – of a piston and cylinder, positioned on the rod. An element ensuring synchronous feeding of vacuum into the cavity of an extracted traction line and pressure into the cavity of an introduced traction line could be a gear mated with cogs of two rods. As each of two gears is coupled only with its pair of traction lines, the bending of the tube's end is performed in two stages. The cross-piece with a management lever, whose central part has a movable connection with the body of the desk node of control bloc, but ends are attached to four rods, pistons and cylinders, ensures simultaneous bending of the tube's end in any direction.

A system for intraction and extraction of biopsy forceps includes sources of pressure and vacuum, which are connected through a cock to the cavity of the biopsy channel, the entrance to which is sealed with a seal of biopsy forceps, at the distal end of which there is a piston of the biopsy channel. In addition the biopsy forceps have an intensifier of traction lines and contain a flexible hermetic tube, which is connected to sources of pressure and vacuum, but the distal end of the tube and traction lines finishes with a cylinder and a piston respectively. The unit piston/cylinder is possible to replace with a segment of sylphone, the distal end of which is connected to traction lines.

Cocks, feeding pressure into the invaginator and mechanism of tube's introduction have to be placed in the pedal node of the control bloc of the endoscopic tube, but the others - in the desk node.

The graphic materials illustrate the essence of invention, where on the fig. 1 is represented the endoscope with disposable cartridge for invagination, where: a - handle-shaped control bloc; b - distal part of endoscopic tube with mounted cartridge; c - longitudinal section of cartridge; d, e, f - enlarged fragments of fig.1c. On fig. 2 is shown the system of extraction-intraction of traction lines when the distal end of an endoscopic tube is in direct position, where: a - position of system elements comprised in control bloc; b - enlarged fragment of fig. 2a; c - distal part of tube with "bared" system elements (vertical arrows show the top-bottom of endoscopic tube); d – enlarged fragment of fig. 2c. On fig. 3 is represented the system of extraction-intraction of traction lines when the end of an endoscopic tube is bent downwards, where: a - position of elements contained in control bloc; b - enlarged fragment of fig. 3a; c - distal part of endoscopic tube with "bared" elements (horizontal arrows show the direction of traction lines motion); d, e - enlarged fragments of fig. 3c. On fig. 4 are represented: a - control bloc and design of new endoscope; b - cross-piece with lever, rods, pistons and cylinders; c – construction of a mechanism for introduction of endoscopic tube into cartridge; d - system of intraction and extraction of biopsy forceps; e – extraction and intraction system of biopsy forceps.

09509377-082800

Specification of numerical markings of figs. 1-4 given at the end of the description is practically similar to graphic materials of the prototype. A novel endoscope includes endoscopic tube 3 with control bloc 2 and communication branch. Air-duct 15 and cock 17 positioned on control bloc 2 or in pedal, connect source of working pressure with opening 21 into the cavity of seal 13, which communicates with cavity 14 of shell 22. The distal part of shell 22 is commensurable in relation to length and diameter to uneverted part of invaginator 23, but the proximal part – to the compressed spring 10. Everted end 12 of invaginator 23 is connected to shell 22 by ring 16. Invaginator 23 has narrowings and widenings 24, as well as gap 25 with distal condom 26. Ends of distal 26 and proximal 27 condoms and corresponding to them places of tube 3 have areas 28 for interconnection and hermetization. Seal 29 on end 7 of invaginator 23 separates cavity 14 from cavity 25, which communicates with the intestinal cavity. A distancer 30 prevents deformation of seal 29 by spring 10. Ends of compressed spring 10 are based on distancer 30 and stop 11 at the end 28 of condom 26. Stop 11, in its turn, is positioned on the projection 31 of shell 22. The distal end of condom 26 ends with tip 6 with channels 32 for washing of protective glass 33 and blowing-up of intestines, as well as an element for connection to endoscopic tube 3. On the border of narrow and broad parts of shell 22 there is an area of intermediate diameter with indented elastic ring 34 for fixation of compressed spring 10. Channel 35 of anal dilator 19 is used for decompression of intestines during intubation. In the tube 3, besides the enumerated, there are elastic tubes 36, 37 comprising springs 38, 39 and traction lines 40, 41. Tubes 36, 37 are connected to springs 38, 39 with thread 42. Near mechanism 43 for bending the distal end of tube 3, ends of tubes 36, 37 are closed with plugs 44, which also connect springs 38, 39 with traction lines 40, 41. Proximal ends of tubes 36, 37 are connected with sources 45 of excess pressure and vacuum. Proximal ends of traction lines 40, 41 are connected with their manual extractors-intractors 46, but the latter - with element 47 which ensures synchronous feeding of vacuum into the cavity of traction line 40 which is being extracted and of pressure into the cavity of traction line 41 which is being introduced. Endoscopic tube 3 has internal pleats 48 of external cover, air-duct 49 with two openings 50 for vacuum fixation of condoms 26, 27 to tube 3 and also has removable sleeve gasket 51. Control bloc 2 has cock 52 of air-duct 49. Seal 13 is hermetically connected to mechanism 53 for introduction of endoscopic tube 3. Mechanism 53 for introduction of tube 3 is operated by pedal 54 but lever 55 realizes bending of tubes end. Cylinder 56, two pistons 57, distancers 58 and elastic tube 59 limit cavity 60, which is connected with source of pressure by means of cock in pedal 54. Cavity 61 comprises return spring 62 and is connected with vacuum by means of cock in pedal 54. Seal 64 and nut 65 are mounted on biopsy forceps 63, but piston 66 is positioned at their distal end. Seat for seal 64 and nut 65 is located at entry 67 to biopsy channel, which is positioned with cock 68 on control bloc 2. Sylphone 69, which serves as source of pressure and vacuum in pneumatic intensifier of traction line of biopsy forceps, can be combined with a handle of biopsy forceps 63.



After the patient has been placed on an endoscopic table a cartridge is oiled and introduced into the rectum and its ampoule is examined as if with a rigid rectoscope. The pressure in cavity 14 is raised by pressing cock 17 thus freeing distancer 30 from coupling with fixator 34 and shell 22. Thereby spring 10 is released and it is possible to proceed with invagination of tube 3. Eversion of invaginator 23 and introduction of tube 3 into the colon occurs under working pressure in cavity 14 at the moments of pressing pedal 54. During endoscopy intestines are to be distended. Gas into intestines is constantly supplied through gas/liquid channel of tube 3 and through channel 32 of tip 6 thus preventing intestinal content of getting under protective glass 33. Gas evacuation from intestines occurs through channel 35 of anal dilator 19.

As during colonoscopy tube 3 repeats all natural flexures of the colon its extubation must not be accelerated. Anal dilator 19 through which extubation is to be conducted eliminates unpleasant sensations caused by this process.

The most practical important version of the invention is a colonoscope with endoscopic tube 3 without biopsy channel. A disposable cartridge ensures an available to all and atraumatic transportation of tube 3 in the colon, condoms 26, 27 protect the patient from infections seated in endoscopic tube 3, but tube 3 - from getting contagious during endoscopy. Ergonomics of handling such colonoscope also makes it available to any physician: during endoscopy a physician in sedentary position, watches the screen, presses pedal cock 17 with one foot, pedal 54 with another, the right hand controls lever

For biopsy a cartridge with tip 6, without glass 33 is used. Having exhausted the possibility of manual insertion of forceps 63, it is necessary by means of seal 64 and nut 65 to hermetize entry 67 into the biopsy channel and connect it by means of cock 68 to the source of pressure. Further insertion of forceps 63 is performed by their manual intraction and due to pressure of liquid or gas on piston 66, but extraction – by switching cock 68 in the position «vacuum» and manual extraction of forceps 63. Due to location of source 69 of pressure and vacuum of traction line intensifier in the handle of forceps, taking of biopate is made as previously - approach of rings ensures movement of the traction line inwards, but detachment - extraction of the traction line.

- 1 - eyepiece (fig. of the prototype only);
- 2 - control bloc with communication branch;
- 3 – endoscopic tube;
- 4 - everted part of invaginator (fig. of the prototype only);
- 5 - source of working pressure in cavity 14 (fig. of the prototype only);
- 6 - tip of endoscopic tube 3;
- 7 - uneverted end of invaginator 23;
- 8,9 – rings at the end 7 of invaginator (fig. of the prototype only);
- 10 - compressed spring;
- 11 - stop for spring 10;
- 12 - everted end of invaginator 23;
- 13 – proximal seal of tube 3;
- 14 - cavity of everted part 4 of invaginator 23;
- 15 – air-duct for feeding working pressure into cavity 14;
- 16 - ring, fixing end 12 of invaginator 23;
- 17- cock of air-duct 15;
- 18 - manometer (fig. of the prototype only);
- 19 - anal dilator;
- 20 - rectum (fig. of the prototype only);
- 21 – air-duct 15 opening on tube 3;
- 22 - shell of cartridge for invagination;
- 23 - invaginator formed in a compact flexible cylinder;
- 24 - narrowings and widenings of cylinder of invaginator 23;
- 25 - gap (cavity) between cylinder of invaginator 23 and condom 26;
- 26 - distal condom of tube 3;
- 27 - proximal condom of tube 3;
- 28 - areas on tube 3 and at the ends of condoms 26, 27 for their hermetic connection;

- 29 – distal seal between tube 3 and end 7 of invaginator 23;
- 30 - distancer between spring 10 and invaginator 23 comprising seal 29;
- 31 - projection on shell 22 for stop 11;
- 32 - channel in tip 6;
- 33 - protective glass of tip 6;
- 34 - elastic ring, fixing spring 10 in compressed state;
- 35 - channel in anal dilator 19;
- 36 - lower elastic tube of extractor-intractor of traction lines;
- 37 - upper elastic tube of extractor-intractor of traction lines;
- 38 - lower spring of extractor-intractor of traction lines;
- 39 - upper spring of extractor-intractor of traction lines;
- 40 – lower traction line of extractor-intractor of traction lines;
- 41 – upper traction line of extractor-intractor of traction lines;
- 42 - thread fixing elastic tubes 36, 37 to springs 38, 39;
- 43 – mechanism for bending of distal end of tube 3;
- 44 - plug closing tubes 36, 37 and connecting springs 38, 39 with traction lines 40, 41;
- 45 - sources of pressure and vacuum;
- 46 - manual extractors-intractors of traction lines 40, 41;
- 47 – element for extraction-intraction of one or two pairs of traction lines;
- 48 - pleats of external cover of tube 3;
- 49 – air-duct into cavity of condoms 26, 27;
- 50 - distal and proximal openings of air-duct 49 on tube 3;
- 51 - sleeve gasket;
- 52 – air-duct 49 cock on control bloc 2;
- 53 –mechanism for insertion of endoscopic tube 3;
- 54 – pedal for switching on mechanism 53;
- 55 - lever of element 47, made in a shape of cross-piece;
- 56 - cylinder of mechanism 53;
- 57- pistons of cylinder 56;
- 58 – distancers between pistons 57;
- 59 - elastic tube, attached to pistons 57;
- 60 - hermetic cavity, enclosed by elastic tube 59 and pistons 57;
- 61 - hermetic cavity, enclosed by seal 13 and distal piston 57;
- 62 - spring returning pistons 57 to home position;
- 63 - biopsy forceps;
- 64 - seal of entry 67 into biopsy channel;
- 65 - nut, fixing seal 64;
- 66 - piston of biopsy forceps;
- 67 - entry into biopsy channel;
- 68 - cock feeding pressure or vacuum into biopsy channel;
- 69 - source of pressure and vacuum connected with cavity of biopsy forceps 63.

003280 226050

1. An endoscope with a disposable cartridge for invagination of an endoscopic tube and biopsy in flexuous channels, incorporating: - a source of light; - sources of pressure and vacuum; - biopsy forceps; - an endoscopic tube with a control block and a communication branch containing inwardly light and image transmission elements, a liquid or gas feeding channel, a biopsy channel, two pairs of closely wound springs with traction lines which pairwise connect the mechanism for bending the distal end to manual extractors of traction lines located in the control block, but externally a spring mounted on the tube, an invaginator, a tip, a seal, an anal dilator, differs in that the invaginator is tightly set in layers in the shape of a cylinder placed with a gap to the endoscopic tube.
2. The endoscope as defined in claim 1 differs in that the invaginator in the form of a compact hollow cylinder is formed of different forms short layers of a thin-walled eversible tube compressed in longitudinal and transverse directions arranged at different angles and has narrowings of an external and widenings of internal diameters.
3. The endoscope as defined in claim 1 or 2 differs in that it is supplied with a disposable cartridge consisting of a shell with a projection at proximal end in which are located the invaginator, a spring, a spring fixator, a spring distancer in which a distal seal of the endoscopic tube fastened at the uneverted end of the invaginator is placed, a condom of the distal part of the endoscopic tube connected to a spring stop and tip with elements for hermetic fastening to the endoscopic tube, at that the proximal seal of the endoscopic tube with an anal dilator having a channel in the wall is located at the shell, but the everted end of the invaginator is fastened at the distal end of shell.
4. The endoscope as defined in claim 3 differs in that the endoscopic tube has transverse pleats of its external cover turned inwards and the areas for air-tight fixation of condoms' ends, as well as two air-ducts with cocks, whereof the larger one communicates through its lateral opening with the cavity of the proximal seal of the endoscopic tube, but the smaller - with the condoms' cavity.
5. The endoscope as defined in any preceding claim differs in that the proximal end of the cartridge for invagination joins the endoscopic tube introduction mechanism made in the shape of a cylinder with two pistons which are interconnected with distancers and the elastic tube, but the cavity between them is connected to the pressure and vacuum sources, at that the cavity between the proximal seal of the endoscopic tube and the distal piston comprises the spring, which returns the pistons to their home position and is connected to vacuum and pressure sources.
6. The endoscope as defined in any preceding claim differs in that it is supplied with an extraction-intraction system of traction lines with hydro-manual drive for controlling the distal end of the endoscopic tube, including pressure and vacuum sources which are linked to elastic tubes cavities comprising liquid and springs with traction lines, at that tubes are fixed to springs with a thread but the springs are made with steps and at the distal end are joined with traction lines, connected in control block with manual extractors-intractors of traction lines, which, in their turn, are joined with elements for synchronous vacuum feeding into the cavity of the manually extracted traction line and excess pressure into the cavity of the introduced traction line.

00509377 032300

- [illegible]

## Abstract

The present invention pertains to the field of medicine and may be used for carrying out biopsies in the serpinginous channels. This invention more precisely relates to an endoscope that comprises an invagination device in the shape of a compact cylender, wherein said cylinder is separated by a gap from the endoscopic tube and has an outer diameter with periodically narrowing sections as well as an inner diameter with periodically widening sections. The endoscope also includes a rod extraction/introduction system for bending the distal end of the endoscopic tube. This endoscope further includes a cartridge in the shape of a sleeve for receiving the condom of the distal part of the endoscopic tube as well as a spring. One end of the invagination device is turned inside out and is connected to the distal end of the sleeve which is covered with a seal, wherein said invagination device also includes an anal dilator and an endoscopic tube nozzle. The endoscope further includes a table unit, control pedals, a mechanism for supplying the endoscopic tube as wel as a cylinder with a piston for introducing biopsy prongs and for sampling biopsy material in the serpiginous channels.

09509377.082300

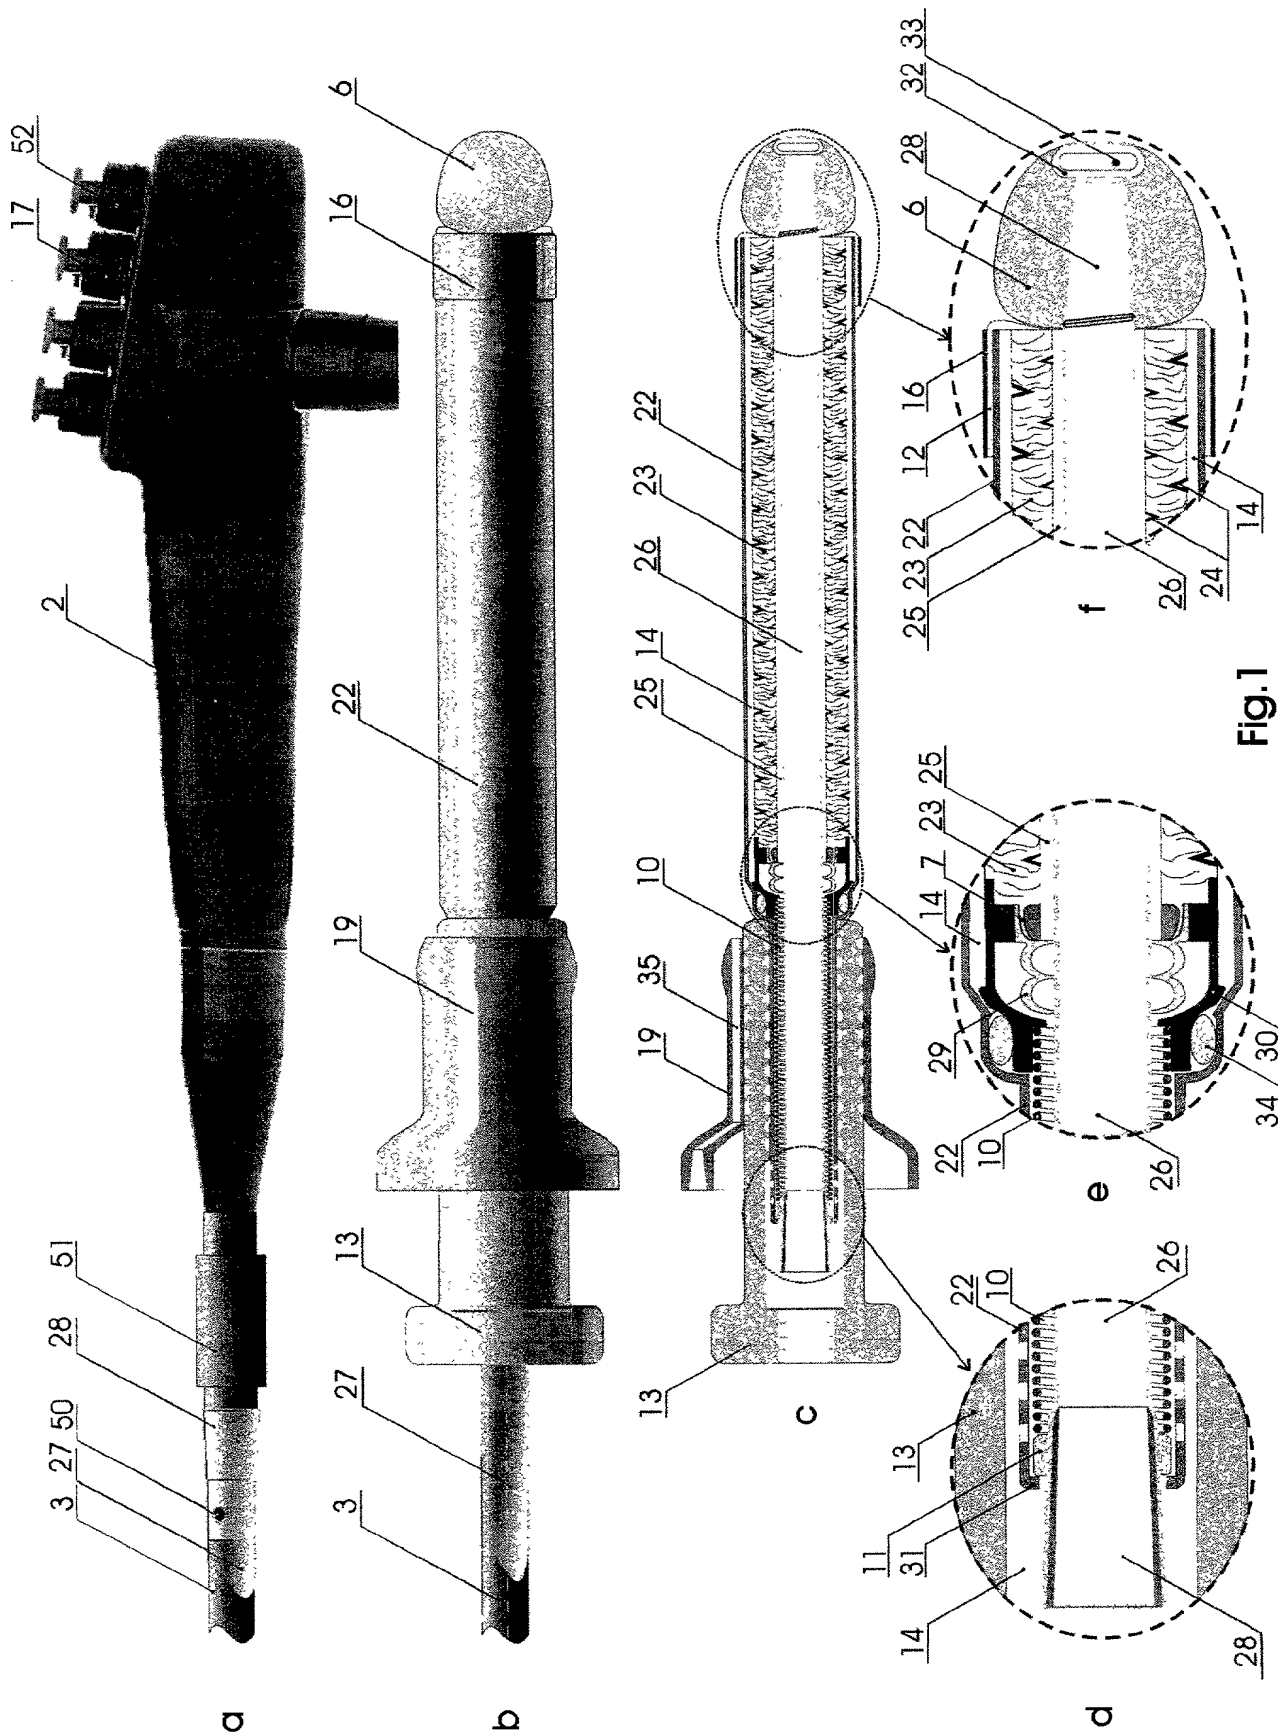


Fig.1

2/4

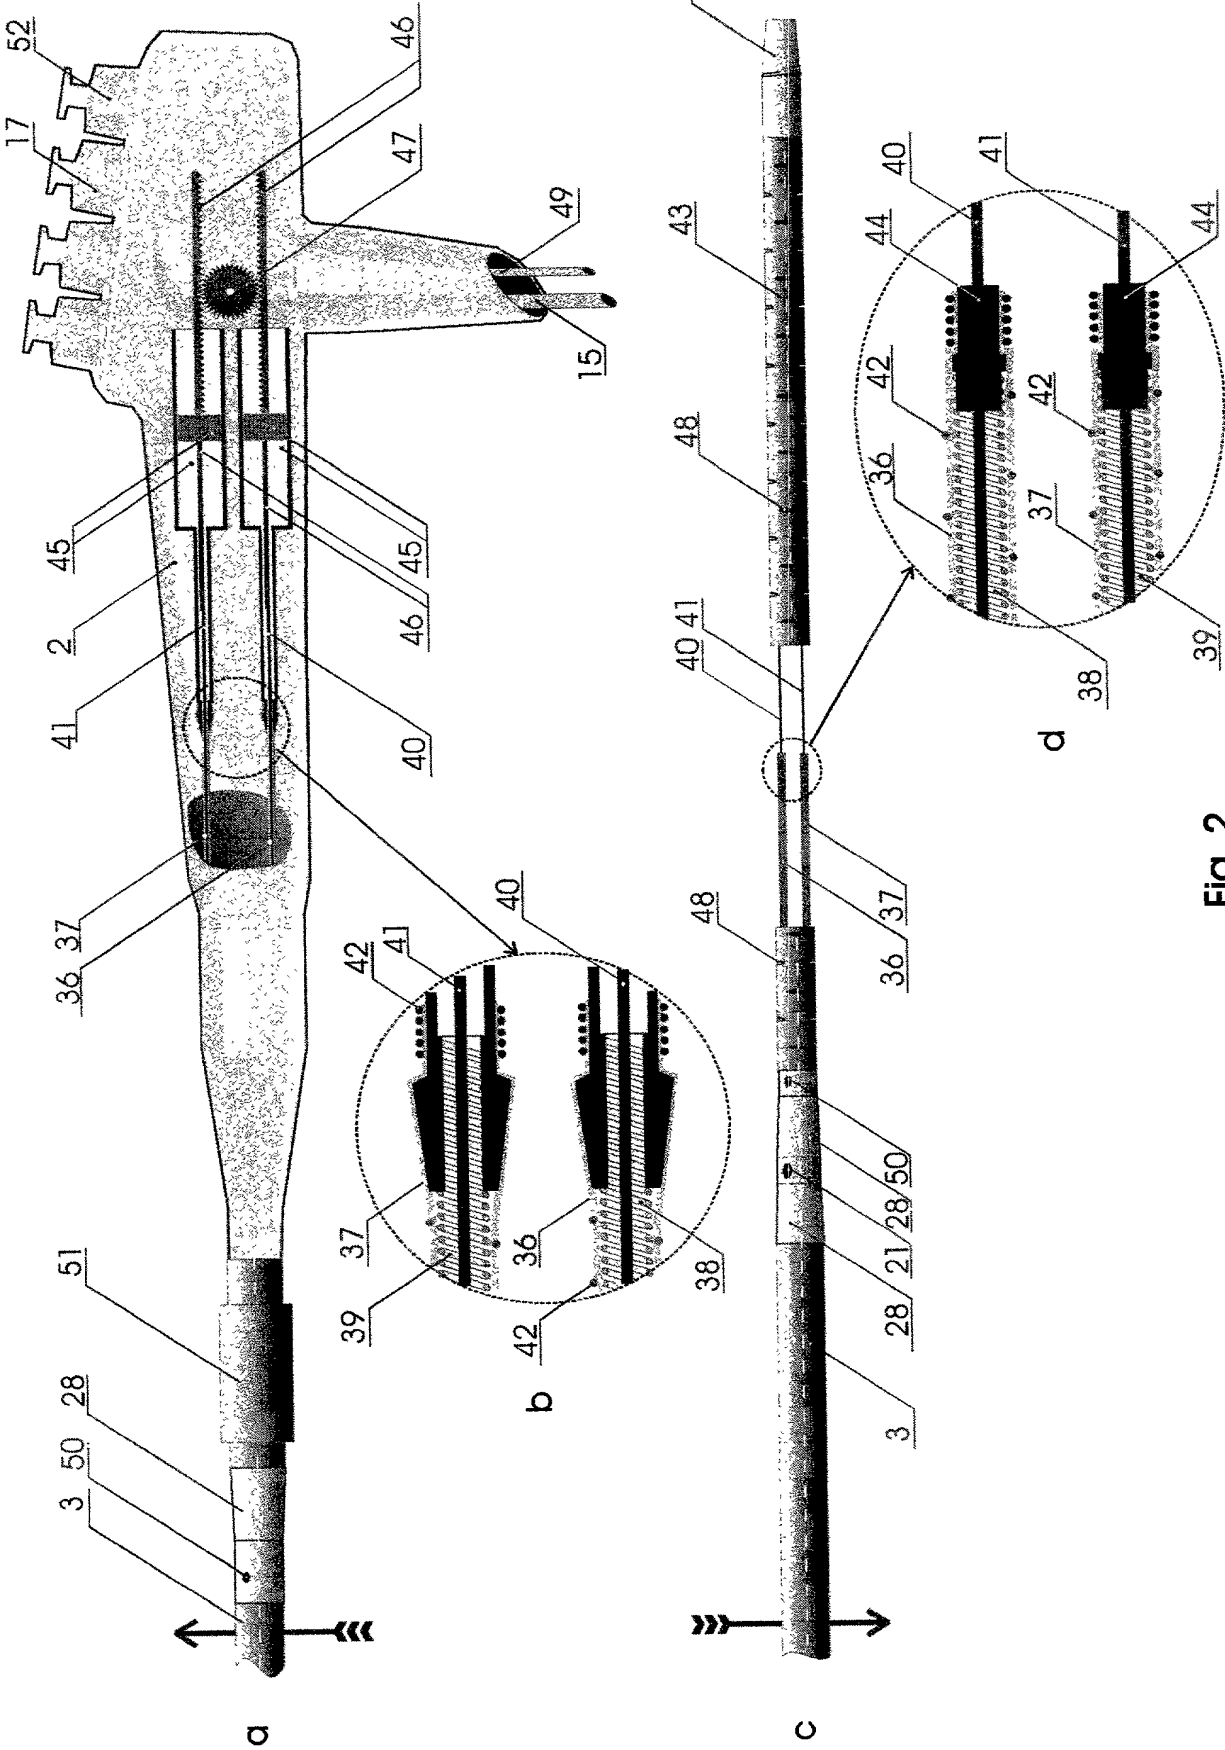


Fig. 2



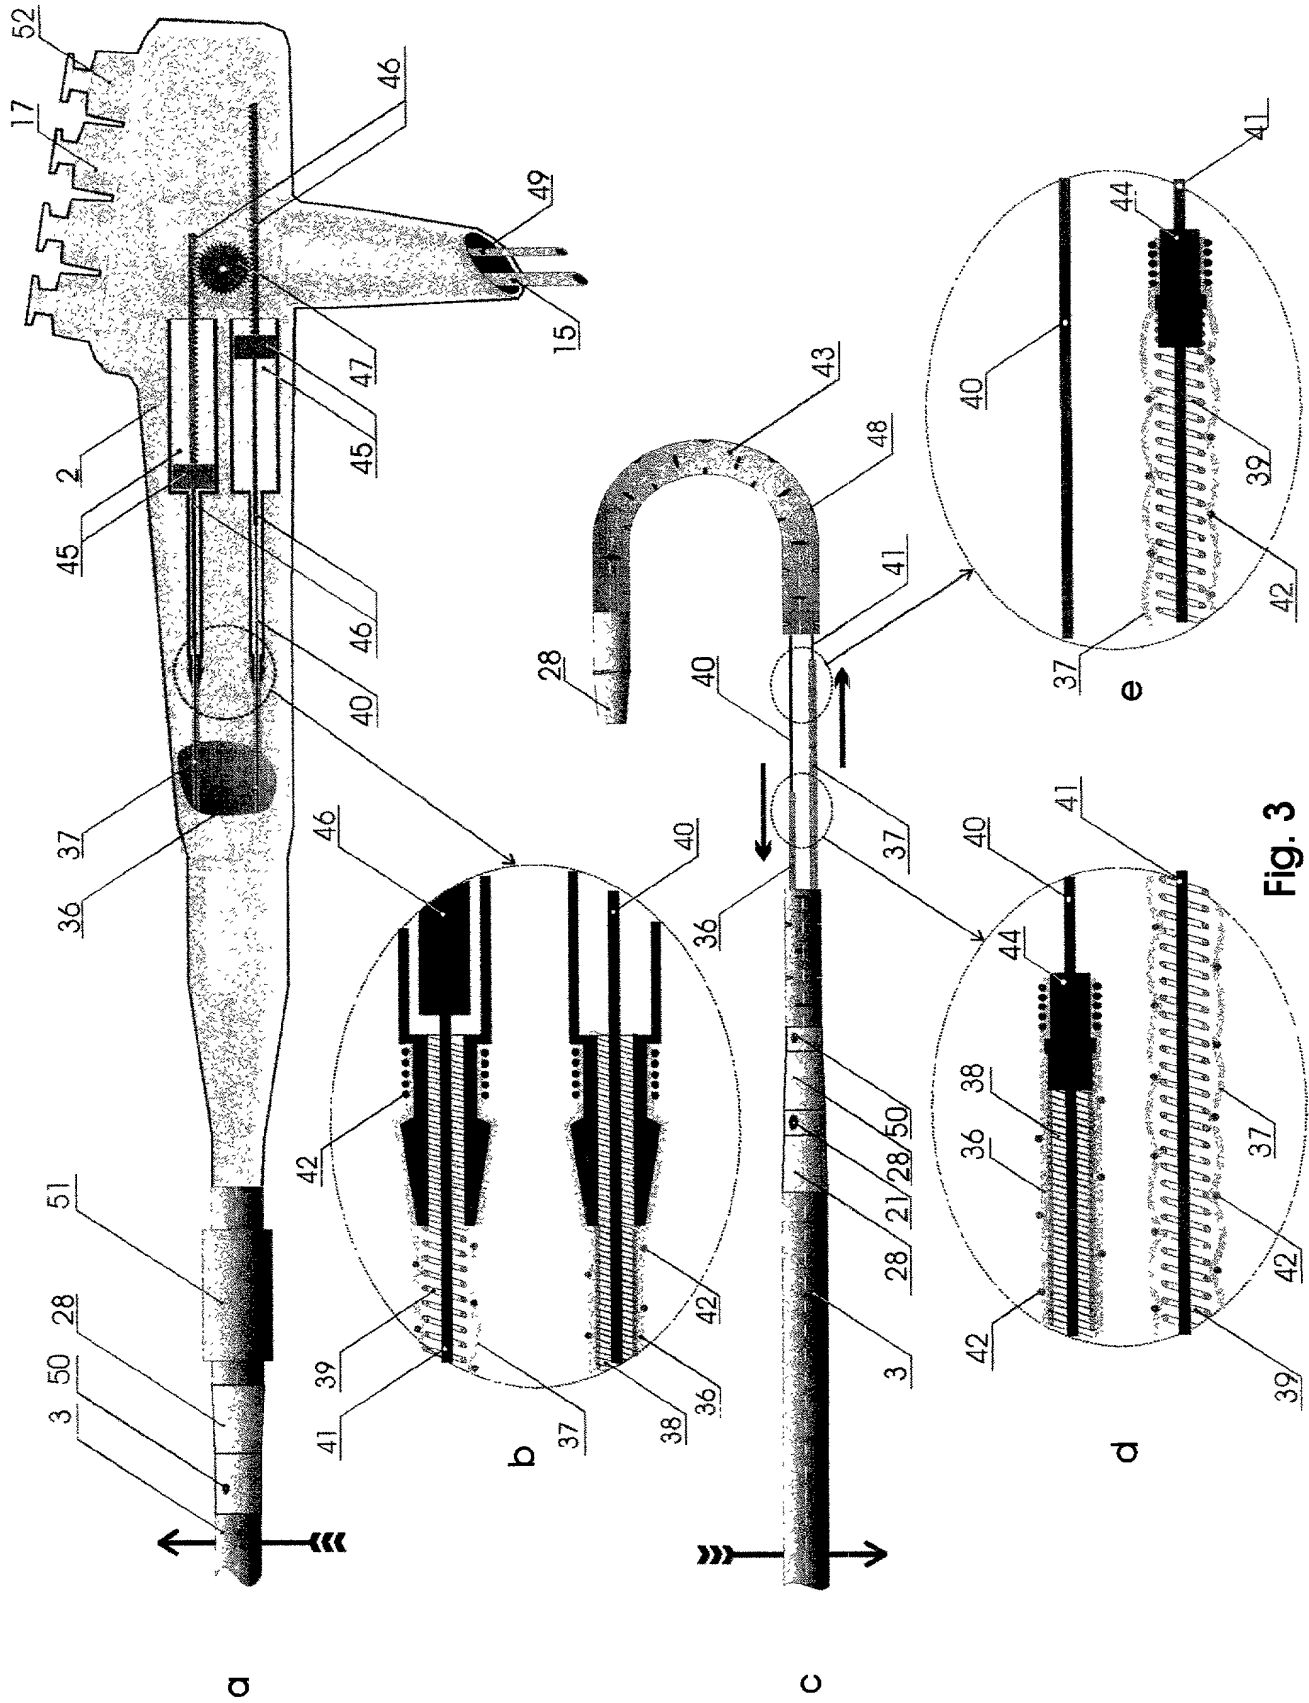


Fig. 3

4/4

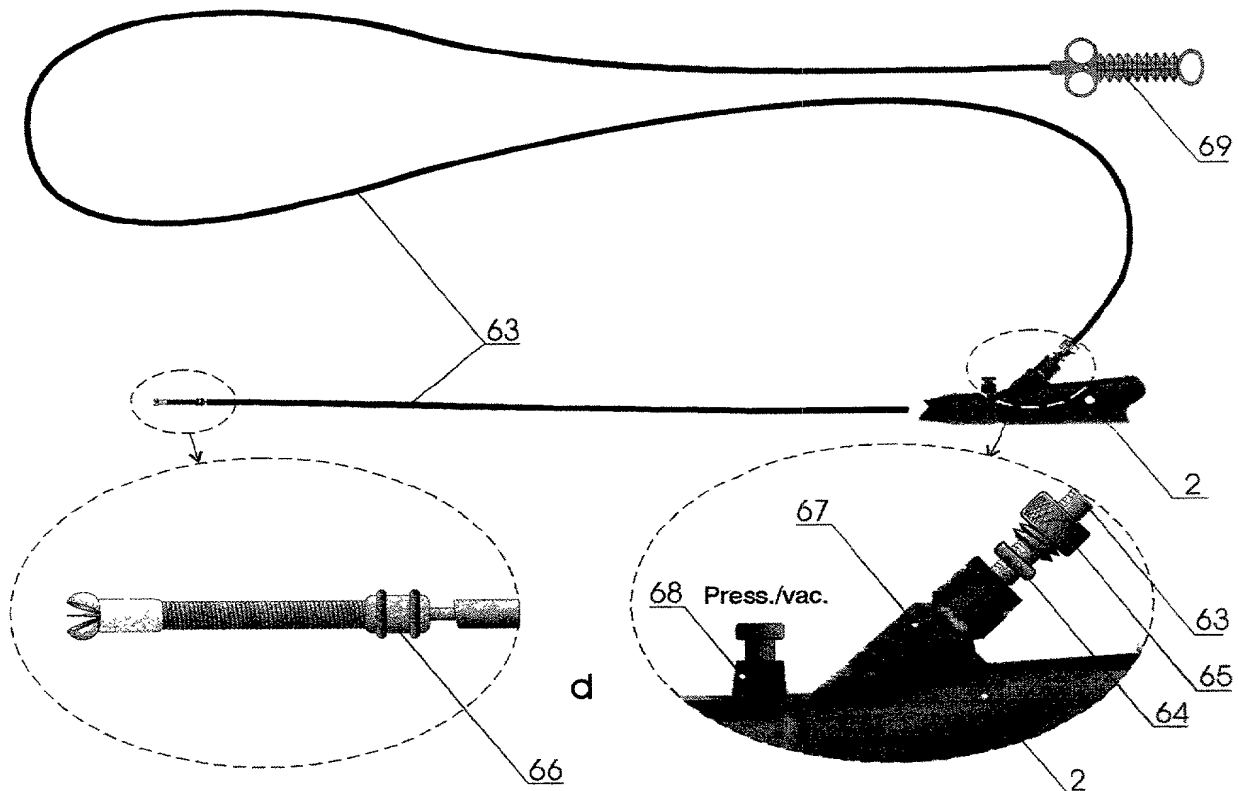
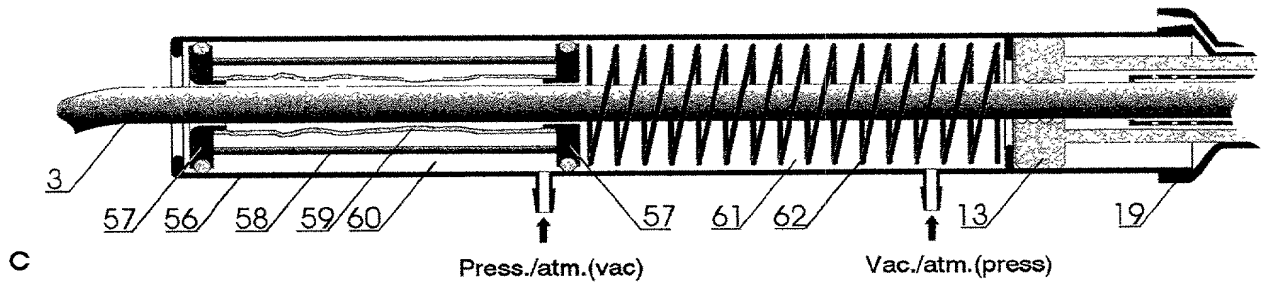
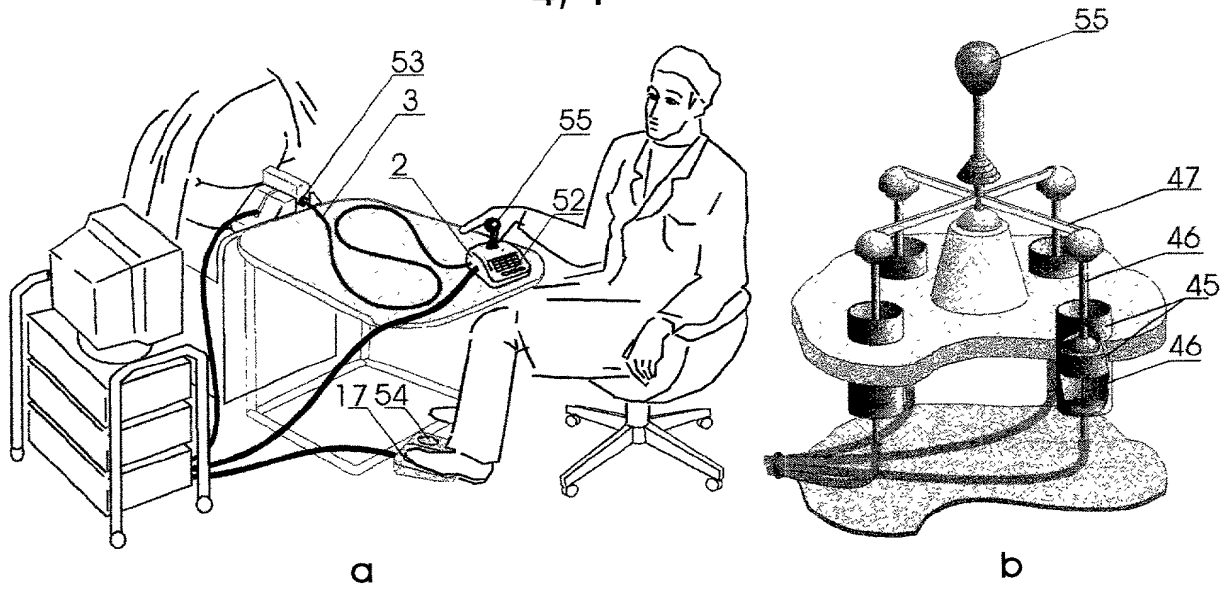


Fig. 4

Please type a plus sign (+) inside this box → **+**

PTO/SB/01 (12-97)

Approved for use through 9/30/00. OMB 0651-0032

Patent and Trademark Office: U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

<b>DECLARATION FOR UTILITY OR DESIGN PATENT APPLICATION</b> <b>(37 CFR 1.63)</b>  <input checked="" type="checkbox"/> Declaration Submitted with Initial Filing <b>OR</b> <input type="checkbox"/> Declaration Submitted after Initial Filing (surcharge (37 CFR 1.16 (e)) required)	<b>Attorney Docket Number</b>	
	<b>First Named Inventor</b>	<b>Sergey Matasov</b>
	<b>COMPLETE IF KNOWN</b>	
	<b>Application Number</b>	/
	<b>Filing Date</b>	
	<b>Group Art Unit</b>	
	<b>Examiner Name</b>	

As a below named inventor, I hereby declare that:

My residence, post office address, and citizenship are as stated below next to my name.

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled:

**Endoscope with single-use cartridge for the invagination of endoscopic tube**

the specification of which (Title of the Invention)

☐ is attached hereto  
**OR**

☒ was filed on (MM/DD/YYYY) **10/02/1998** as United States Application Number or PCT International

Application Number **PCT/LV98/00006** and was amended on (MM/DD/YYYY) **01/10/2000** (if applicable).

I hereby state that I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment specifically referred to above.

I acknowledge the duty to disclose information which is material to patentability as defined in 37 CFR 1.56.

I hereby claim foreign priority benefits under 35 U.S.C. 119(a)-(d) or 365(b) of any foreign application(s) for patent or inventor's certificate, or 365(a) of any PCT international application which designated at least one country other than the United States of America, listed below and have also identified below, by checking the box, any foreign application for patent or inventor's certificate, or of any PCT international application having a filing date before that of the application on which priority is claimed.

Prior Foreign Application Number(s)	Country	Foreign Filing Date (MM/DD/YYYY)	Priority Not Claimed	Certified Copy Attached?	
				YES	NO
P-97-190 P-98-188 i.c. 1522466	LATVIA LATVIA USSR	10/03/1997 09/23/1998 08/21/1978	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
			<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

☐ Additional foreign application numbers are listed on a supplemental priority data sheet PTO/SB/02B attached hereto:

I hereby claim the benefit under 35 U.S.C. 119(e) of any United States provisional application(s) listed below.

Application Number(s)	Filing Date (MM/DD/YYYY)	<input type="checkbox"/> Additional provisional application numbers are listed on a supplemental priority data sheet PTO/SB/02B attached hereto.

[Page 1 of 2]

Burden Hour Statement: This form is estimated to take 0.4 hours to complete. Time will vary depending upon the needs of the individual case. Any comments on the amount of time you are required to complete this form should be sent to the Chief Information Officer, Patent and Trademark Office, Washington, DC 20231. **DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Assistant Commissioner for Patents, Washington, DC 20231.**

Please type a plus sign (+) inside this box → ☐

PTO/SB/01 (12-97)

Approved for use through 9/30/00. OMB 0651-0032

Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

## DECLARATION — Utility or Design Patent Application

I hereby claim the benefit under 35 U.S.C. 120 of any United States application(s), or 365(c) of any PCT international application designating the United States of America, listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States or PCT international application in the manner provided by the first paragraph of 35 U.S.C. 112. I acknowledge the duty to disclose information which is material to patentability as defined in 37 CFR 1.56 which became available between the filing date of the prior application and the national or PCT international filing date of this application.

U.S. Parent Application or PCT Parent Number	Parent Filing Date (MM/DD/YYYY)	Parent Patent Number (if applicable)
PCT/LV 98/00006	10/02/1998	

☐ Additional U.S. or PCT international application numbers are listed on a supplemental priority data sheet PTO/SB/02B attached hereto.

As a named inventor, I hereby appoint the following registered practitioner(s) to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith:

☐ Customer Number  OR  
☐ Registered practitioner(s) name/registration number listed below

Place Customer  
Number Bar Code  
Label here

Name	Registration Number	Name	Registration Number

☐ Additional registered practitioner(s) named on supplemental Registered Practitioner Information sheet PTO/SB/02C attached hereto.

Direct all correspondence to: ☐ Customer Number  OR ☒ Correspondence address below

Name	Sergey Matasov				
Address	Ranka dambis 7/1 - 55				
Address					
City	Riga	State		ZIP	LV1048
Country	LATVIA	Telephone	+371 7601489	Fax	+ 371 7601489

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under 18 U.S.C. 1001 and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

Name of Sole or First Inventor:		<input checked="" type="checkbox"/> A petition has been filed for this unsigned inventor			
Given Name (first and middle (if any))		Family Name or Surname			
Sergey		Matasov			
Inventor's Signature				Date	03/20/2000
Residence: City	Riga	State		Country	Latvia
Post Office Address	Slokas 33				
Post Office Address	LVX				
City	Riga	State		ZIP	LV1048
				Country	LATVIA

☐ Additional inventors are being named on the \_\_\_\_\_ supplemental Additional Inventor(s) sheet(s) PTO/SB/02A attached hereto